



Your complimentary  
use period has ended.  
Thank you for using  
PDF Complete.


[Click Here to upgrade to](#)

[Unlimited Pages and Expanded Features](#)

0828\_multisizer\yFB30\_400uMGal\yFB30\_400uMGal\_1\_02.#M3

Preference file: C:\MSI\Default.pri (modified)  
Group ID: yFB30\_400uMGal  
Sample ID: 1  
Run number: 2  
Electrolyte: ISOTON II  
Aperture diameter: 30  $\mu\text{m}$  Kd: 38.899  
Aperture current: 400  $\mu\text{A}$  Gain: 8  
Size bins: 300 from 0.6  $\mu\text{m}$  to 18  $\mu\text{m}$   
Sigma: 31,106 (Coincidence corrected)  
Count > 0.719  $\mu\text{m}$ : 30,003 Coincidence corrected: 31,109  
Coincidence correction: 3.7%  
Control mode: Total Count 30,000  
Elapsed time: 59.32 seconds  
Acquired: 16:45 28 Aug 2019  
Dilution Factor: 500  
Electrolyte volume: 10 mL

### Differential Number

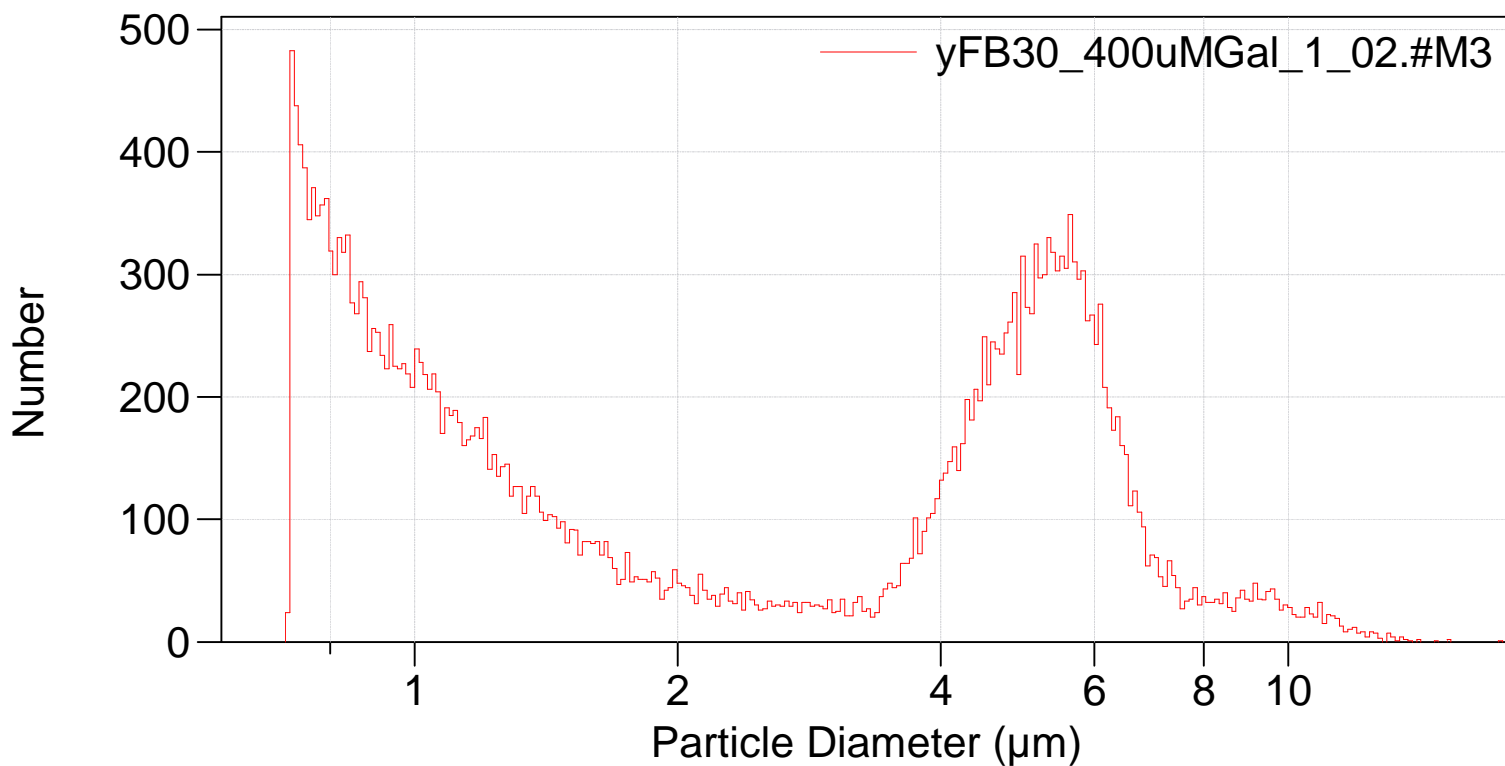

**Sigma = 31,106**